



Designation: D4404 – 18

Standard Test Method for Determination of Pore Volume and Pore Volume Distribution of Soil and Rock by Mercury Intrusion Porosimetry¹

This standard is issued under the fixed designation D4404; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope*

1.1 This test method covers the determination of the pore volume and the pore volume distributions of soil and rock by the mercury intrusion porosimetry method. The range of apparent diameters of pores for which this test method is applicable is fixed by the operating pressure range of the testing instrument. This range is typically between apparent pore entrance diameters of about 400 μm and 2.5 nm (0.0025 μm). Larger pores must be measured by another method.

1.2 Mercury intrusion porosimetry is useful only for measuring pores open to the outside of a soil or rock fragment; mercury intrusion porosimetry will not give the volume of any pores completely enclosed by surrounding solids. This test method will give only the volume of intrudable pores that have an apparent diameter corresponding to a pressure within the pressurizing range of the testing instrument.

1.3 Mercury intrusion may involve the application of high pressures to the specimen. This may result in a temporary or permanent alteration or both in the pore geometry. Generally, soils and rocks are composed of comparatively strong solids and are less subject to these alterations than certain other materials. However, the possibility remains that the use of this test method may alter the natural pore volume distribution that is being measured.

1.4 **Warning**—Mercury has been designated by EPA and many state agencies as a hazardous material that can cause central nervous system, kidney and liver damage. Mercury, or its vapor, may be hazardous to health and corrosive to materials. Caution should be taken when handling mercury and mercury-containing products. See the applicable product Material Safety Data Sheet (MSDS) for details and EPA's website (<http://www.epa.gov/mercury/faq.htm>) for additional information. Users should be aware that selling mercury or mercury-containing products or both into your state may be prohibited by state law.

¹ This test method is under the jurisdiction of ASTM Committee D18 on Soil and Rock and is the direct responsibility of Subcommittee D18.06 on Physical-Chemical Interactions of Soil and Rock.

Current edition approved Feb. 1, 2018. Published March 2018. Originally approved in 1984. Last previous edition approved in 2010 as D4404–10. DOI: 10.1520/D4404-18.

1.5 **Units**—The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard. Reporting of test results in units other than SI, such as cgs, shall not be regarded as nonconformance with this test method.

1.6 All observed and calculated values shall conform to the guidelines for significant digits and rounding established in Practice D6026.

1.6.1 The procedures used to specify how data are collected/recorded and calculated in this standard are regarded as the industry standard. In addition, they are representative of the significant digits that generally should be retained. The procedures used do not consider material variation, purpose for obtaining the data, special purpose studies, or any considerations for the user's objectives; and it is common practice to increase or reduce significant digits of reported data to be commensurate with these considerations. It is beyond the scope of these test methods to consider significant digits used in analysis methods for engineering data.

1.7 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.* For specific precaution statements, see Section 8.

1.8 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

2. Referenced Documents

- 2.1 *ASTM Standards*:²
[D653 Terminology Relating to Soil, Rock, and Contained Fluids](#)
[D3740 Practice for Minimum Requirements for Agencies](#)

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

*A Summary of Changes section appears at the end of this standard

3. Terminology

3.1 For definitions of common technical terms used in this standard, refer to Terminology **D653**.

3.2 Definitions of Terms Specific to This Standard:

3.2.1 *apparent pore diameter*—the diameter of a pore that is assumed to be cylindrical and that is intruded at a pressure, P , given by the equation in **13.1**.

3.2.2 *inter-specimen pores*—those pores between particles when they are packed together and that are intruded during the test.

3.2.3 *intra-specimen pores*—those pores lying within the exterior outlines of the individual soil and rock fragments.

3.2.4 *intruded pore volume*—the corrected volume of mercury intruded during the test.

4. Summary of Test Method

4.1 When a liquid does not wet a porous solid, it will not enter the pores in the solid by capillary action. The non-wetting liquid (mercury in this test method) can be forced into the pores by the application of external pressure. The size of the pores that are intruded is inversely proportional to the applied pressure. The diameter of the pores filled can be calculated from this applied pressure as described in Section 13, Calculations.

4.2 The volume of the intruded pores is determined by measuring the volume of mercury forced into them at various pressures. A single determination involves increasing the pressure, either continuously or step-wise, and recording the measured intruded volume at various pressures.

4.2.1 The sample is contained in a sample cell frequently called a penetrometer. The sample is contained within a sealed bowl to which a small capillary is attached. The space in the penetrometer not occupied by the sample is first evacuated and then filled with mercury. One end of the penetrometer is open and sealed to the pressure system of the instrument. Pressure applied to the open end of the penetrometer capillary is then used to force the mercury into the pores, with larger pores filling at lower applied pressures, and smaller pores filling at higher applied pressures.

4.3 Additional information about the pore structure of the material may be determined by recording of the extrusion profile for the sample. This is performed by recording the cumulative quantity of mercury contained within the sample as pressure is reduced, again either continuously or step-wise.

4.4 Commercially available instruments include software for controlling sample evacuation, filling of sample penetrometer with mercury, pressurization of the sample according to a programmed scheme, allowance for equilibration of the pressure, recording of the pressure and amount of mercury intruded into the sample, and calculation of summary results.

5. Significance and Use

5.1 This test method is intended for use in determining the volume and the volume distribution of pores in soil and rock with respect to the apparent diameter of the entrances of the pores. In general, both the size and volume of the pores affects the performance of soil and rock. Thus, the pore volume distribution is useful in understanding soil and rock performance and in identifying a material that can be expected to perform in a particular manner (**1, 2**).³

5.2 The intrusion process to determine the volume of a pore proceeds from the outside of a specimen toward its center. Comparatively large interior pores can exist that have smaller outside openings as the only means of access. Mercury intrusion porosimetry will incorrectly register the entire volume of these “ink-bottle” pores as having the apparent diameter of the smaller access pores. In a test specimen, exterior specimen pores can exist in addition to intra-specimen pores (see **3.2** for definitions). The inter-fragment pores will vary in size and volume depending on the size and shape of the soil or rock fragments and on the manner in which the fragments are packed together. It is possible that some exterior specimen pores can have the same apparent diameter as some intra-specimen pores. When this occurs, this test method cannot distinguish between them. Thus, the test method yields an intruded pore volume distribution that is in part dependent upon the packing of multifragment specimens. However, most soils and rocks have intra-fragment pores much smaller than the inter-fragment pores. This situation leads to a bi-modal pore size distribution and the distinction between the two classes of pores can then be made (see **Figs. 1 and 2**). The intr-fragment pore concentration is shown to the left of the plot; the inter-fragment concentration is to the right.

NOTE 1—The quality of the result produced by this standard is dependent on the competence of the personnel performing it, and the suitability of the equipment and facilities used. Agencies that meet the criteria of Practice **D3740** are generally considered capable of competent and objective testing/sampling/inspection/etc. Users of this standard are cautioned that compliance with Practice **D3740** does not in itself assure reliable results. Reliable results depend on many factors; Practice **D3740** provides a means of evaluating some of those factors.

6. Apparatus

6.1 *Mercury Intrusion Porosimeter*—A device equipped with a specimen holder capable of containing one or several soil or rock fragments. This specimen holder is frequently called a penetrometer. The porosimeter shall have a means of surrounding the test specimen with mercury at a low pressure, a pressure generator to cause intrusion, pressure transducers, capable of measuring the intruding pressure with an accuracy of at least $\pm 1\%$ throughout the range of pressures over which the pores of interest are being intruded, and a means of measuring intruded mercury volumes to an accuracy of at least $\pm 1 \text{ mm}^3$.

6.2 *Analytical Balance*, with an accuracy of at least $\pm 10^{-6}$ kg (± 1 mg), and readable to at least $\pm 10^{-7}$ kg (± 0.1 mg).

³ The boldface numbers in parentheses refer to the list of references appended to this standard.

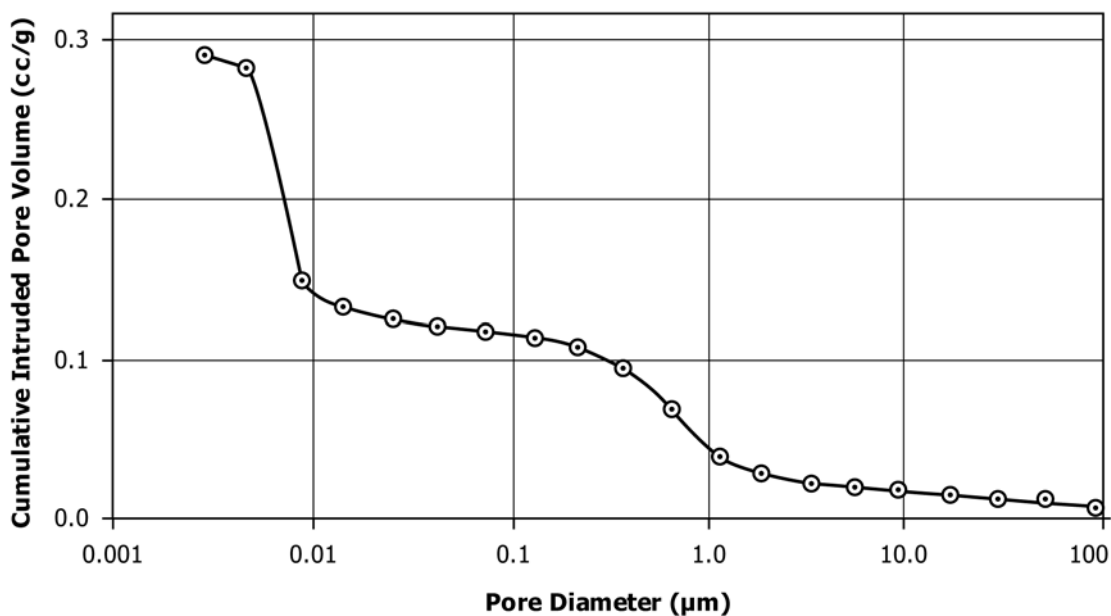


FIG. 1 Example of Cumulative Pore Volume Distribution Plot

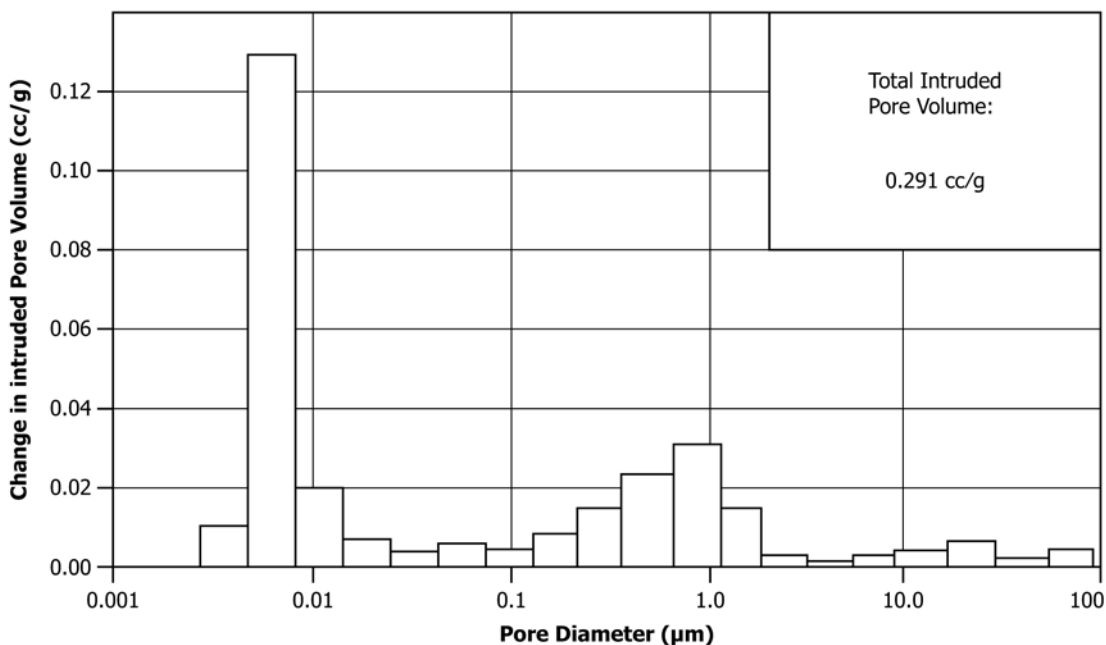


FIG. 2 Example of Differential Pore Volume Distribution Plot

6.3 *Fume Hood*—A ventilated enclosure designed to limit exposure to hazardous/toxic vapors, fumes, or dust by providing a means to move the air away from the user, preferably venting it outside.

6.4 *Thermometric Device*—A thermometric device capable of measuring the temperature range within which the test is being performed readable to 0.5°C or better and having an accuracy of at least ±1°. The thermometric device shall be standardized by comparison to a nationally or internationally traceable thermometric device and shall include at least one

temperature reading within the range of testing. The thermometric device shall be standardized at least once every twelve months.

6.5 *Drying Oven*—Controllable at or above 150 ± 10°C.

7. Reagent

7.1 *Triple-Distilled Mercury*.

7.2 *Purity of Reagents*—Reagent grade chemicals shall be used in all tests. Unless otherwise indicated, it is intended that