



# Standard Test Methods for Determination of the Impact Value (IV) of a Soil<sup>1</sup>

This standard is issued under the fixed designation D5874; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

## 1. Scope\*

1.1 These test methods cover the determination of the Impact Value (IV) of a soil either in the field or a test mold, as follows:

1.1.1 *Field Procedure A*—Determination of IV alone, in the field.

1.1.2 *Field Procedure B*—Determination of IV and water content, in the field.

1.1.3 *Field Procedure C*—Determination of IV, water content, and dry density, in the field.

1.1.4 *Mold Procedure*—Determination of IV of soil compacted in a mold, in the lab.

1.2 The standard test method, using a 4.5 kg (10 lbm) hammer, is suitable for, but not limited to, evaluating the strength of an unsaturated compacted fill, in particular pavement materials, soils, and soil-aggregates having maximum particle sizes less than 37.5 mm (1.5 in.).

1.3 By using a lighter 0.5 kg (1.1 lbm) or 2.25 kg (5 lbm) hammer, this test method is applicable for evaluating lower strength soils such as fine grained cohesionless, highly organic, saturated, or highly plastic soils having a maximum particle size less than 9.5 mm (0.375 in.), or natural turfgrass.

1.4 By using a heavier 10 kg (22 lbm) or 20 kg (44 lbm) hammer, this test method is applicable for evaluating for harder materials at the top end the scales or beyond the ranges of the standard and lighter impact soil testers.

1.5 By performing laboratory test correlations for a particular soil using the 4.5 kg (10 lbm) hammer, IV may be correlated with an unsoaked California Bearing Ratio (CBR) or may be used to infer percentage compaction.

1.6 The values stated SI are to be regarded as the standard. The values stated in parentheses are given for information only.

1.7 All observed and calculated values shall conform to the guidelines for significant digits and rounding established in Practice [D6026](#).

<sup>1</sup> This test method is under the jurisdiction of ASTM Committee [D18](#) on Soil and Rock and is the direct responsibility of Subcommittee [D18.08](#) on Special and Construction Control Tests.

Current edition approved Jan. 1, 2016. Published January 2016. Originally approved in 1995. Last previous edition approved in 2007 as D5874 – 02(2007). DOI: 10.1520/D5874-16.

1.8 For purposes of comparing, a measured or calculated value(s) with specified limits, the measured or calculated value(s) shall be rounded to the nearest decimal or significant digits in the specified limits.

1.8.1 The procedures used to specify how data are collected/recorded or calculated, in this standard are regarded as the industry standard. In addition, they are representative of the significant digits that generally should be retained. The procedures used do not consider material variation, purpose for obtaining the data, special purpose studies, or any considerations for the user's objectives; and it is common practice to increase or reduce significant digits of reported data to be commensurate with these considerations. It is beyond the scope of this standard to consider significant digits used in analysis methods for engineering design.

1.9 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

NOTE 1—The equipment and procedures contained in this test method are similar to those developed by B. Clegg in the 1970s at the University of Western Australia, Nedlands, Australia. Impact Value is also commonly known as Clegg Impact Value (CIV).

## 2. Referenced Documents

2.1 *ASTM Standards*:<sup>2</sup>

[D653 Terminology Relating to Soil, Rock, and Contained Fluids](#)

[D698 Test Methods for Laboratory Compaction Characteristics of Soil Using Standard Effort \(12 400 ft-lbf/ft<sup>3</sup> \(600 kN-m/m<sup>3</sup>\)\)](#)

[D1556 Test Method for Density and Unit Weight of Soil in Place by Sand-Cone Method](#)

[D1557 Test Methods for Laboratory Compaction Characteristics of Soil Using Modified Effort \(56,000 ft-lbf/ft<sup>3</sup> \(2,700 kN-m/m<sup>3</sup>\)\)](#)

[D1883 Test Method for California Bearing Ratio \(CBR\) of Laboratory-Compacted Soils](#)

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, [www.astm.org](http://www.astm.org), or contact ASTM Customer Service at [service@astm.org](mailto:service@astm.org). For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

\*A Summary of Changes section appears at the end of this standard

- [D2167 Test Method for Density and Unit Weight of Soil in Place by the Rubber Balloon Method](#)
- [D2216 Test Methods for Laboratory Determination of Water \(Moisture\) Content of Soil and Rock by Mass](#)
- [D2937 Test Method for Density of Soil in Place by the Drive-Cylinder Method](#)
- [D3740 Practice for Minimum Requirements for Agencies Engaged in Testing and/or Inspection of Soil and Rock as Used in Engineering Design and Construction](#)
- [D4643 Test Method for Determination of Water \(Moisture\) Content of Soil by Microwave Oven Heating](#)
- [D4959 Test Method for Determination of Water \(Moisture\) Content of Soil By Direct Heating](#)
- [D6026 Practice for Using Significant Digits in Geotechnical Data](#)
- [D6938 Test Methods for In-Place Density and Water Content of Soil and Soil-Aggregate by Nuclear Methods \(Shallow Depth\)](#)

3.2.9 *medium impact value (IV/M), n*—the IV derived from using a 2.25 kg (5 lbm) mass hammer 50 mm (2.0 in.) in diameter free falling 450 mm (18 in.).

#### 4. Summary of Test Method

4.1 The test apparatus is placed on the material to be tested either in a mold or on naturally occurring or compacted soil in the field. The hammer is raised to a set height and allowed to free fall. The instrumentation of the test apparatus displays a value in tens of gravities (*g*) of the peak deceleration of the hammer's impact as recorded by an accelerometer fitted to the top of the hammer body. A total of four blows of the hammer are applied on the same spot to determine the IV for each test performed.

4.2 A lighter hammer of 0.5 kg (1.1 lbm) or 2.25 kg (5 lbm) may be used for softer conditions or fragile materials instead of the 4.5 kg (10 lbm) standard hammer to determine the IV. When used the resulting value is termed the Light Impact Value (IV/L) for the 0.5 kg (1.1 lbm) hammer or Medium Impact Value (IV/M) for the 2.25 kg (5 lbm) hammer.

4.3 A larger, heavier hammer of 10 kg (22 lbm) or 20 kg (44 lbm) may be used instead of the 4.5 kg (10 lbm) standard hammer to determine the IV for harder conditions or to test through a larger zone both horizontally and vertically. When used, the resulting value is termed the Heavy Medium Heavy Impact Value (IV/HMH) for the 10 kg (22 lbm) hammer or Heavy Impact Value (IV/H) for the 20 kg (44 lbm) hammer.

#### 5. Significance and Use

5.1 Impact Value, as determined using the standard 4.5 kg (10 lbm) hammer, has direct application to design and construction of pavements and a general application to earthworks compaction control and evaluation of strength characteristics of a wide range of materials, such as soils, soil aggregates, stabilized soil and recreational turf. Impact Value is one of the properties used to evaluate the strength of a layer of soil up to about 150 mm (6 in.) in thickness and by inference to indicate the compaction condition of this layer. Impact Value reflects and responds to changes in physical characteristics that influence strength. It is a dynamic force penetration property and may be used to set a strength parameter.

5.2 This test method provides immediate results in terms of IV and may be used for the process control of pavement or earthfill activities where the avoidance of delays is important and where there is a need to determine variability when statistically based quality assurance procedures are being used.

5.3 This test method does not provide results directly as a percentage of compaction but rather as a strength index value from which compaction may be inferred for the particular moisture conditions. From observations, strength either remains constant along the dry side of the compaction curve or else reaches a peak and declines rapidly with increase in water content slightly dry of optimum water content. This is generally between 95 and 98 % maximum dry density (see Fig. 1 and Fig. 2). An as-compacted target strength in terms of IV may be designated from laboratory testing or field trials as a strength to achieve in the field as the result of a compaction process for a

### 3. Terminology

#### 3.1 Definitions:

3.1.1 Except as listed in 3.2, all definitions are in accordance with Terminology D653.

#### 3.2 Definitions of Terms Specific to This Standard:

3.2.1 *as-compacted target IV, n*—the desired strength, in terms of IV, to be achieved in the field for a particular material and construction process, at the as-compacted moisture condition. This may also be referred to as the *as-compacted target strength*.

3.2.2 *dried-back target IV, n*—the desired strength, in terms of IV, to be achieved in the field for a particular material and construction process prior to continuing with a subsequent layer, or sealing, or opening to traffic, after moisture has left the system through evaporation and/or drainage. This may also be referred to as the *dried-back target strength*.

3.2.3 *heavy impact value (IV/H), n*—the IV derived from using a 20 kg (44 lbm) mass hammer 130 mm (5 in.) in diameter free falling 300 mm (12 in.).

3.2.4 *heavy medium heavy impact value (IV/HMH), n*—the IV derived from using a 10 kg (22 lbm) mass hammer 130 mm (5 in.) in diameter free falling 300 mm (12 in.).

3.2.5 *impact soil tester, n*—testing apparatus used to obtain an IV of a soil.

3.2.6 *impact value (IV), n*—the value expressed in units of tens of gravities (*g*) and reported to the nearest whole number derived from the peak deceleration of a 4.5 kg (10 lbm) instrumented compaction hammer 50 mm (2.0 in.) in diameter free falling 450 mm (18 in.).

3.2.7 *in-service target IV, n*—the desired strength, in terms of IV, to be achieved in the field for a particular material and construction process once the road is opened to traffic and has reached equilibrium. This may also be referred to as the *in-service target strength*.

3.2.8 *light impact value (IV/L), n*—the IV derived from using a 0.5 kg (1.1 lbm) mass hammer 50 mm (2.0 in.) in diameter free falling 300 mm (12 in.).

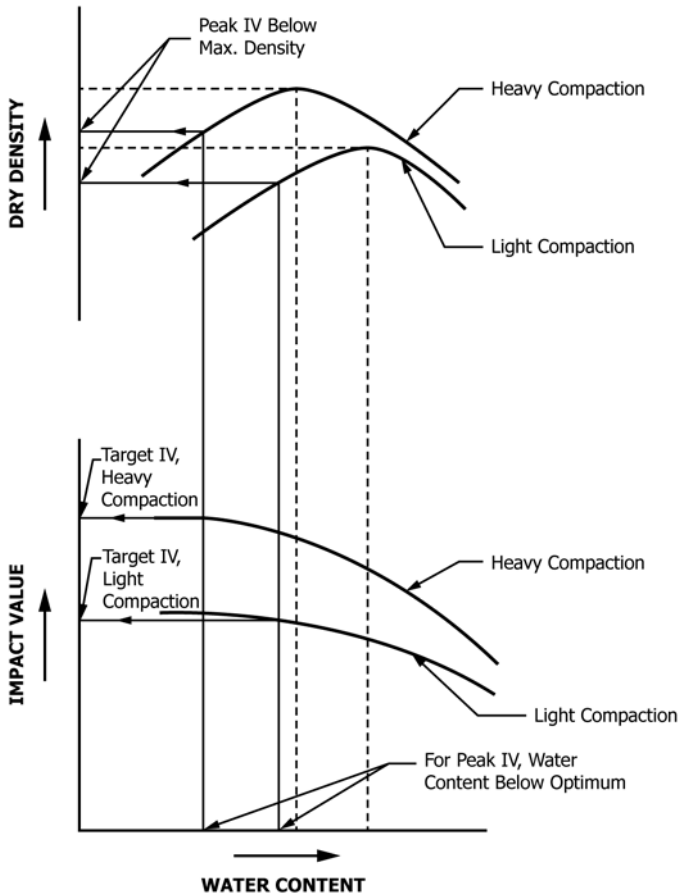


FIG. 1 Illustration of Target IV for Material with No Peak

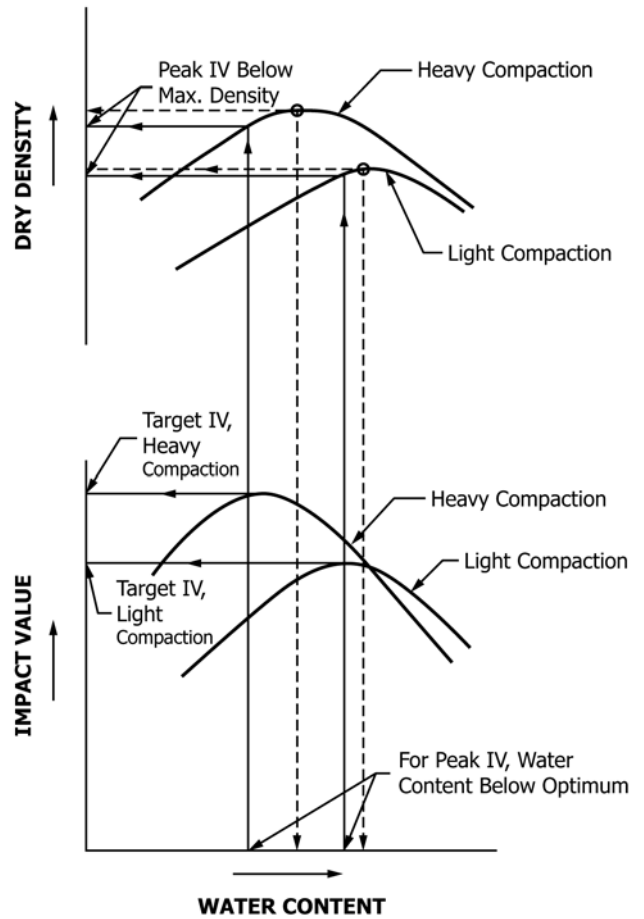


FIG. 2 Illustration of Target IV for Material with Pronounced Peak

desired density and water content. If testing is performed after compaction when conditions are such that the water content has changed from the critical value, determination of the actual water content by laboratory testing enables the field density to be inferred from regression equations using IV, density and water content.

NOTE 2—Impact Value may be used as a means to improve the compaction process by giving instant feedback on roller efficiency, uniformity, confirming the achievement of the target strength, and by inference the achieved density. When inferring density from IV, however, it should be considered as only indicative of density. Where strict acceptance on a density ratio basis is required, test methods that measure density directly shall be used.

5.4 This test method may be used to monitor strength changes during a compaction process or over time due to seasonal, environmental or traffic changes.

NOTE 3—For in-place soil strength evaluation where there may be a dry and hard surface layer (crust), testing both the crust and the underlying layer may be required.

5.5 The standard instrument is based on a 4.5 kg (10 lbm) compaction hammer using a 450 mm (18 in.) drop height. The hammer has been equipped with an accelerometer and instrumented using a peak hold electronic circuit to read the peak deceleration on impact. The circuitry is filtered electronically to remove unwanted frequencies and the peak deceleration is displayed in units of ten gravities (g) with the output below units of ten gravities truncated.

5.6 The peak deceleration on which IV is derived represents the area under the deceleration versus time curve which for most soils may be assumed as half a sinusoid. Applying double integration provides first the time velocity relationship and second, the time penetration relationship. As force is also directly related to deceleration, the IV therefore, represents both stress and penetration and may be taken as a direct measurement of stiffness or strength (see Fig. 3).

5.7 Impact Value may be correlated with an unsoaked CBR.

5.8 Impact Value may be expressed as a hammer modulus, analogous with elastic modulus or deformation modulus.

5.9 The light hammer uses the same accelerometer and instrumentation as the standard hammer. The smaller mass of 0.5 kg (1.1 lbm) results in more sensitivity for lower strength materials compared to the standard mass; that is, the zero to 100 IV scale is expanded with this lighter hammer mass and provides more definition on softer materials. To avoid confusion, the IV of the light hammer is notated as IV/L.

5.10 Light Impact Value has applications for recreation turf hardness evaluation, where the condition of the surface affects ball bounce characteristics, the performance or injury potential to participants, and where more sensitivity compared to the standard hammer is required or an imprint left by the 4.5 kg (10 lbm) hammer or other test methods is undesirable, such as on a golf putting green.