



Standard Test Method for Rubber—Compositional Analysis by Thermogravimetry (TGA)¹

This standard is issued under the fixed designation D6370; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This test method provides a thermogravimetric (TGA) technique to determine the amounts of organics (oil, polymer), carbon black and ash (filler) in a rubber compound.

1.2 The amount of plasticizer/oil may be determined separately using Test Method [D297](#).

1.3 This test method utilizes previously calibrated, manual or computer assisted TGA instrumentation.

1.4 The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

1.5 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 ASTM Standards:²

[D297](#) Test Methods for Rubber Products—Chemical Analysis

[D1566](#) Terminology Relating to Rubber

[D4483](#) Practice for Evaluating Precision for Test Method Standards in the Rubber and Carbon Black Manufacturing Industries

[D6085](#) Practice for Sampling in Rubber Testing—Terminology and Basic Concepts

[E473](#) Terminology Relating to Thermal Analysis and Rheology

[E1953](#) Practice for Description of Thermal Analysis and Rheology Apparatus

¹ This test method is under the jurisdiction of ASTM Committee [D11](#) on Rubber and is the direct responsibility of Subcommittee [D11.11](#) on Chemical Analysis.

Current edition approved Aug. 1, 2014. Published November 2014. Originally approved in 1999. Last previous edition approved in 2009 as D6370 – 99 (2009). DOI: 10.1520/D6370-99R14.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

3. Terminology

3.1 Definitions:

3.1.1 The definitions relating to rubber appearing in Terminology [D1566](#) shall be considered applicable to this test method.

3.1.2 The terminology relating to sampling appearing in Practice [D6085](#) shall be considered applicable to this test method.

3.1.3 The definitions for thermal analysis appearing in Terminology [E473](#) shall be considered applicable to this test method.

3.1.4 The description of thermal analysis equipment appearing in Practice [E1953](#) shall be considered applicable to this test method.

3.2 Definitions of Terms Specific to This Standard:

3.2.1 *ash*, *n*—nonvolatile additives (fillers), such as zinc oxide, talc, etc.

3.2.2 *carbon black*, *n*—carbon black.

3.2.3 *organics*, *n*—rubber (polymer), noncarbon black organic additives, such as oil, plasticizer, antioxidants, etc.

4. Summary of Test Method

4.1 The mass of the rubber test sample, heated at a controlled, specified rate in a controlled, specified environment is recorded as a function of temperature. The mass loss over the specified temperature range provides a compositional analysis of the sample.

5. Significance and Use

5.1 This test method is intended for use in quality control, material screening, and related problem solving where a compositional analysis, or comparison to a known material, is desired.

5.2 The parameters described are guidelines and may be altered to suit the analysis of other rubber compounds.

5.3 This test method is not suitable for rubber compounds containing filler materials which decompose in the temperature range of 50 to 800°C, for example, CaCO_3 , $\text{Al}(\text{OH})_3(3\text{H}_2\text{O})$, etc. Analysis of compounds containing fillers of this type requires knowledge of the filler type and some correction for mass loss.

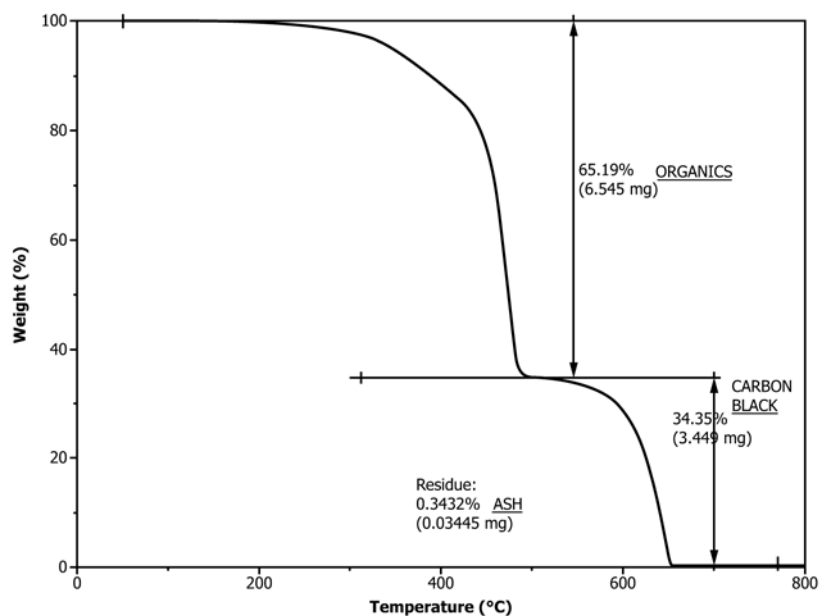


FIG. 1 Typical Thermogram

6. Apparatus

6.1 *Thermogravimetric Analyzer*—A system of related instruments that are capable of continuously weighing a test sample, at a sensitivity of $\pm 2 \mu\text{g}$, and recording the change in mass of the test sample under atmospheric control over a specified temperature range.

7. Reagents and Materials

7.1 An inert compressed gas, such as argon or nitrogen, and a reactive gas, such as air or oxygen.

7.2 Compressed gases must be 99.99 % minimum purity.

7.3 The inert purge gas must not contain more than $10 \mu\text{g/g}$ oxygen.

8. Calibration

8.1 Calibrate the apparatus, according to the prescribed procedures or appropriate operating manual, at the heat (temperature) and purge gas flow rates to be used.

9. Procedure

9.1 Place a small piece, 10 to 12 mg, of the rubber test sample into the platinum pan of the calibrated Thermogravimetric Analyzer (TGA).

9.2 Apply a $75 \text{ cm}^3/\text{min}$, or the manufacturer's recommended flow, argon or nitrogen purge.

9.3 Heat to 50°C and allow the instrument to equilibrate for a minimum of 2 min.

9.4 Heat from 50 to 560°C at $10^\circ\text{C}/\text{min}$.

9.5 Cool to 300°C and allow the temperature to equilibrate for a minimum of 2 min.

9.6 Change the purge gas to air or oxygen and purge at $75 \text{ cm}^3/\text{min}$ or the manufacturer's recommended flow.

9.7 Heat from 300 to 800°C at $10^\circ\text{C}/\text{min}$.

10. Calculation

10.1 Record the percent mass loss for organics, carbon black, and ash as follows (see Fig. 1):

10.2 For EPDM, NR, PE, PP and SBR:

Component	% Mass Loss
Organics	50 to 550°C (nitrogen)
Carbon black	310 to 790°C (air)
Ash	Residue at 790°C

10.3 For CPE, CR, NBR and PVC:

Component	% Mass Loss
Organics	50 to 550°C (nitrogen) + 310 to 560°C (air)
Carbon black	560 to 790°C (air)
Ash	Residue at 790°C

11. Report

11.1 Report the following information:

11.1.1 Identification of the test sample.

11.1.2 *Percents*—organics, carbon black, and ash found, each to the nearest 0.1 %.

12. Precision and Bias³

12.1 This precision and bias section has been prepared in accordance with Practice D4483. Please refer to this practice for terminology and other statistical calculation details.

12.2 The precision results in this precision and bias section give an estimate of the precision of this test method with the materials (rubbers, etc.) used in the particular interlaboratory test program (ITP) as described below. The precision parameters should not be used for acceptance or rejection testing of

³ Supporting data have been filed at ASTM International Headquarters and may be obtained by requesting Research Report RR:D11-1089.