



Standard Test Method for Instrumented Impact Testing of Metallic Materials¹

This standard is issued under the fixed designation E2298; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reappraisal. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reappraisal.

1. Scope*

1.1 This test method establishes the requirements for performing instrumented Charpy V-Notch (CVN) and instrumented Miniaturized Charpy V-Notch (MCVN) impact tests on metallic materials. This method, which is based on experience developed testing steels, provides further information (in addition to the total absorbed energy) on the fracture behavior of the tested materials. Minimum requirements are given for measurement and recording equipment such that similar sensitivity and comparable total absorbed energy measurements to those obtained in Test Methods E23 and E2248 are achieved.

1.2 The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 ASTM Standards:²

- A370 Test Methods and Definitions for Mechanical Testing of Steel Products
- E4 Practices for Force Verification of Testing Machines
- E23 Test Methods for Notched Bar Impact Testing of Metallic Materials
- E177 Practice for Use of the Terms Precision and Bias in ASTM Test Methods
- E691 Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method
- E2248 Test Method for Impact Testing of Miniaturized Charpy V-Notch Specimens

¹ This test method is under the jurisdiction of ASTM Committee E28 on Mechanical Testing and is the direct responsibility of Subcommittee E28.07 on Impact Testing.

Current edition approved Oct. 1, 2015. Published December 2015. Originally approved in 2009. Last previous edition approved in 2013 as E2298–13a. DOI: 10.1520/E2298-15.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

2.2 ISO Standard:

ISO 14556 Steel—Charpy V-notch Pendulum Impact Tests—Instrumented Test Method³

3. Terminology

3.1 *Definitions*—The symbols and definitions applicable to instrumented impact testing are indicated in Table 1.

4. Summary of Test Method

4.1 This test method prescribes the requirements for instrumented CVN and MCVN impact tests in accordance with Test Methods E23 and E2248. The E23 and E2248 tests consist of breaking by one blow from a swinging pendulum, under conditions defined hereafter, a specimen notched in the middle and supported at each end. In order to establish the impact force-displacement diagram, it is necessary to instrument the striker with strain gages⁴ and measure the voltage as a function of time during the impact event. The voltage-time curve is converted to the force-time curve through a suitable static calibration. The force-displacement relationship is then obtained by double integration of the force-time curve. The area under the force-displacement curve corresponds to the energy absorbed by the specimen during the test.

4.2 Force-displacement curves for different steels and different temperatures can vary even though the areas under the curves and the absorbed energies are identical. If the force-displacement curves are divided into a number of characteristic parts, various phases of the test with characteristic forces, displacements, and energies can be deduced. These characteristic values provide additional information about the fracture behavior of the specimen.

4.3 Application of instrumented test data to the evaluation of material behavior is the responsibility of the user of this test method.

5. Significance and Use

5.1 Instrumented impact testing provides an independent measurement of the total absorbed energy associated with

³ Available from American National Standards Institute (ANSI), 25 W. 43rd St., 4th Floor, New York, NY 10036, <http://www.ansi.org>.

⁴ This test method refers to strikers instrumented with strain gages. However, the use of piezoelectric load cells or accelerometers is not excluded, provided their temperature sensitivity is properly accounted for.

*A Summary of Changes section appears at the end of this standard

TABLE 1 Symbols and Designations Related to Instrumented Impact Testing

| Symbol | Definition | Unit |
|----------|--|------------------|
| F_a | Force at end of unstable crack propagation (arrest force) | N |
| F_{gy} | General yield force | N |
| F_m | Maximum force | N |
| F_{bf} | Force at initiation of brittle fracture (unstable crack propagation) | N |
| g | Local acceleration due to gravity | m/s ² |
| h_0 | Initial falling height of the striker | m |
| KV | Absorbed energy measured from the machine dial or encoder | J |
| m | Total effective mass of moving striker | kg |
| s_a | Displacement at end of unstable crack propagation (arrest force) | m |
| s_{gy} | Displacement at general yield | m |
| s_m | Displacement at maximum force | m |
| s_{bf} | Displacement at initiation of brittle fracture | m |
| s_t | Displacement at end of force-displacement curve | m |
| t_0 | Time at the beginning of deformation of the specimen | s |
| v_0 | Initial striker impact velocity | ms ⁻¹ |
| W_a | Partial impact energy from $F = 0$ to $F = F_a$ | J |
| W_{bf} | Partial impact energy from $F = 0$ to $F = F_{bf}$ | J |
| W_m | Partial impact energy from $F = 0$ to $F = F_m$ | J |
| W_t | Total impact energy | J |

fracturing CVN or MCVN specimens for test machines equipped with a dial and/or optical encoder.

5.2 Instrumented impact testing is particularly effective in MCVN testing since the resolution of a calibrated strain-gaged striker does not necessarily decrease with the magnitude of the measured energy.

5.3 In addition to providing an measure of total absorbed energy (W_t), instrumented testing enables the determination of characteristic force, energy, and displacement parameters. Depending on the material and test temperature, these parameters can provide very useful information (in addition to total absorbed energy) on the fracture behavior of materials such as: the temperature which corresponds to the onset of the lower shelf; the temperature which corresponds to the onset of the upper shelf; the pre-maximum force energy (W_m); the post-maximum force energy; the energy associated with shear lip tearing after brittle fracture; the general yield force (F_{gy}); the force at brittle fracture initiation (F_{bf}); the arrest force (F_a). The instrumented data may also be used to highlight test results which should be discarded on the basis of misalignment or other critical test factors.

6. Precautions in Operation of the Machine

6.1 Safety precautions should be taken to protect personnel from electric shock, the swinging pendulum, flying broken specimens, and hazards associated with specimen warming and cooling media. See also 1.3.

7. Apparatus

7.1 The test shall be carried out in accordance with Test Methods E23 or E2248 using a pendulum impact testing machine which is instrumented to determine force-time or force-displacement curves.

7.1.1 For instrumented CVN testing, the use of an instrumented striker conforming to the specifications of ISO 14556

(i.e., 2 mm radius of striking edge) is allowed. Available data (1, 2)⁵ indicate that the influence of striker geometry on instrumented CVN forces is not very significant.

7.2 Force Measurement:

7.2.1 Force measurement is achieved by using an electronic sensor (piezoelectric load cell, strain gage load cell or a force measurement derived from an accelerometer).

7.2.2 The force measuring system (including strain gages, wiring, and amplifier) shall have an upper frequency bound of at least 100 kHz for CVN tests and 250 kHz for MCVN tests. For MCVN tests, if only absorbed energy has to be measured from the curve, an upper frequency limit of 100 kHz is sufficient. The upper frequency bound for the system shall be verified by measurement or analysis. Measurements can be made using a function generator which is wired directly to the strain gage bridge.

7.2.3 The signal shall be recorded without filtering. Post-test filtering, however, is allowed.

7.2.4 Calibration of the recorder and measurement system may be performed statically in accordance with the accuracy requirements given below. It is recommended that the force calibration be performed with the striker attached to the pendulum assembly. The strain gage signal conditioning equipment, cables, and recording device shall be used in the calibration. In most cases, a computer is used for data acquisition and the calibration shall be performed with the voltage read from the computer. The intent is to calibrate through the electronics and cables which are used during actual testing. Force is applied to the striker by using a suitable load frame with a load cell verified in accordance with Practices E4.

7.2.4.1 The static linearity and hysteresis error of the built-in, instrumented striker, including all parts of the measurement system up to the recording apparatus (printer, plotter, etc.), shall be within $\pm 2\%$ of the recorded force, between 50 and 100 % of the nominal force range, and within $\pm 1\%$ of the full scale force value between 10 and 50 % of the nominal force range (see Fig. 1).

7.2.4.2 The instrumented striker system shall be calibrated to ensure accurate force readings are obtained over the nominal force range which will be encountered in testing. The strain gaged system shall be designed to minimize its sensitivity to non-symmetric loading.

7.2.5 Calibration shall be performed if the instrumented striker has undergone dismantling or repair, unless it can be shown that removal of the striker from the test machine, and subsequent reattachment to the machine, does not affect the calibration. Calibration shall also be performed under the circumstances described below.

7.2.6 *Requirements on Absorbed Energy*—For each test in which the entire force signal has been recorded (i.e., until the force returns to the baseline), the difference between absorbed energy given by the dial and/or optical encoder KV and the total impact energy W_t shall be within 15 % or 1 J, whichever is larger. If this requirement is not met but the difference does not exceed 25 % or 2 J, whichever is larger, force values shall

⁵ The boldface numbers in parentheses refer to the list of references at the end of this standard.

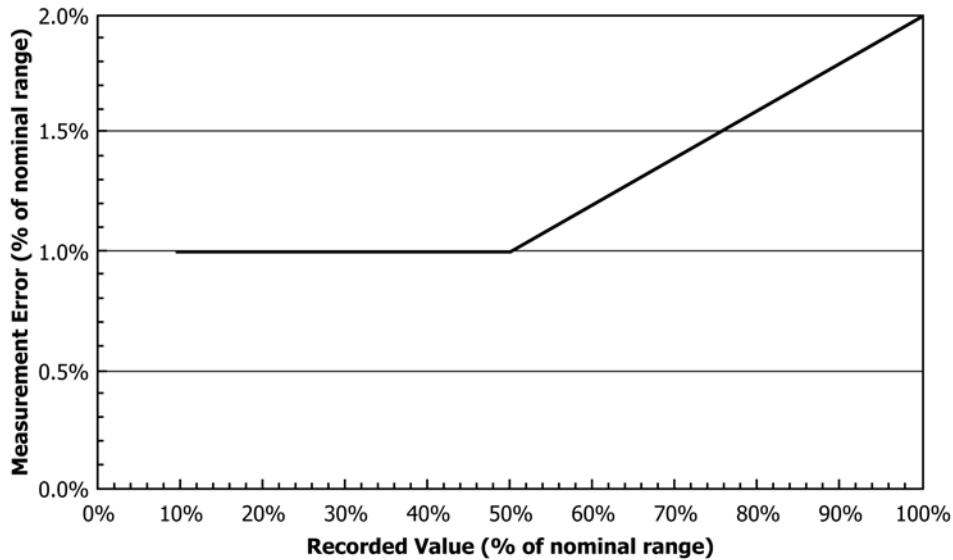


FIG. 1 Allowable Errors in Force Measurements

be adjusted until $KV = W_t$ within 0.01 J (3). If the difference exceeds 25 % or 2 J, whichever is larger, the test shall be discarded and the user shall check and if necessary repeat the calibration of the instrumented striker. If recording of the entire force signal is not possible (for example due to the specimen being ejected from the machine without being fully broken), the user shall demonstrate conformance to the requirements above by testing at least five Charpy specimens of any equivalent material.

NOTE 1—Specimens with certified values of maximum force (F_m) can be tested to verify the accuracy of the force values measured by the instrumented striker. Dynamic impact force verification specimens are available⁶ with certified F_m values of 24.06 kN and 33.00 kN. These values have been established at room temperature through an interlaboratory study (4) involving six international laboratories, see also 13.1.3. The same verification specimens can also be used to verify the absorbed energy scale of the impact machine in accordance with Test Methods E23 at either $-40\text{ °C} \pm 1\text{ °C}$ or room temperature ($21\text{ °C} \pm 1\text{ °C}$).

7.3 Displacement Determination:

7.3.1 Displacement is normally determined by converting a strain gage voltage-time measurement to a force-time measurement. The force-time relationship is proportional to the acceleration as a function of time. Given an assumed rigid striker of mass m , the initial impact velocity v_0 , the time t following the beginning of the deformation at t_0 , and expressing the velocity as a function of time by $v(t)$, the specimen bending displacement $s(t)$ is calculated by double numerical integration as follows:

$$v(t) = v_0 - \frac{1}{m} \int_{t_0}^t F(t) dt \tag{1}$$

⁶ The sole source of supply of the specimens known to the committee at this time is NIST. If interested, email charpy@boulder.nist.gov. If you are aware of alternative suppliers, please provide this information to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee,¹ which you may attend.

$$s(t) = \int_{t_0}^t v(t) dt \tag{2}$$

7.3.2 The initial impact velocity needed to perform the above integrations may be calculated from:

$$v_0 = \sqrt{2gh_0} \tag{3}$$

where:

g = the local acceleration due to gravity, and
 h_0 = the falling height of the striker.

7.3.2.1 Alternatively, the velocity signal registered when the pendulum passes through its lowest position and strikes the specimen can be optically measured directly to determine v_0 .

7.3.3 Displacement can also be determined by non-contacting measurement of the displacement of the striker relative to the anvil using optical, inductive, or capacitive methods. The signal transfer characteristics of the displacement measurement system must correspond to that of the force measuring system in order to make the two recordings synchronous. The displacement measuring system shall be designed for nominal values of up to 30 mm. Linearity errors in the measuring system shall yield measured values to within +2 % in the range 1–30 mm. Measurements between zero and 1 mm may not be sufficiently accurate to determine the displacement. In such cases, it is recommended that the displacement of the specimen be determined from time measurement and the striker impact velocity as indicated in Eq 1 and 2.

7.4 Recording Apparatus:

7.4.1 The minimum data acquisition requirement is a 10-bit analog-digital converter with a minimum sampling rate of 1000 data points per millisecond. However, 12-bit or more is recommended. A minimum storage capacity of 8000 data points is required.