



Designation: D6493 – 11 (Reapproved 2022)

# Standard Test Methods for Softening Point of Hydrocarbon Resins and Rosin Based Resins by Automated Ring-and-Ball Apparatus<sup>1</sup>

This standard is issued under the fixed designation D6493; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

## 1. Scope

1.1 These test methods are intended for determining the softening point of hydrocarbon resins, rosin based resins and similar materials by means of an automated ring-and-ball apparatus. Portions are similar in technical content to the automated-apparatus versions of Test Methods D36, E28, and ISO 4625.

1.1.1 The ring-and-ball softening point of a hydrocarbon resin and rosin based resins may also be determined with lower precision using the manual ring-and-ball softening point procedure in Test Methods E28.

1.2 The values stated in SI units are to be regarded as the standard. The values given in parentheses are for information only.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.*

1.4 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

## 2. Referenced Documents

2.1 *ASTM Standards:*<sup>2</sup>

D36 Test Method for Softening Point of Bitumen (Ring-and-Ball Apparatus)

E1 Specification for ASTM Liquid-in-Glass Thermometers

<sup>1</sup> These test methods are under the jurisdiction of ASTM Committee D01 on Paint and Related Coatings, Materials, and Applications and are the direct responsibility of Subcommittee D01.34 on Pine Chemicals and Hydrocarbon Resins.

Current edition approved Dec. 1, 2022. Published December 2022. Originally approved in 1999. Last previous edition approved in 2015 as D6493 – 11 (2015). DOI: 10.1520/D6493-11R22.

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, [www.astm.org](http://www.astm.org), or contact ASTM Customer Service at [service@astm.org](mailto:service@astm.org). For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

E28 Test Methods for Softening Point of Resins Derived from Pine Chemicals and Hydrocarbons, by Ring-and-Ball Apparatus

E177 Practice for Use of the Terms Precision and Bias in ASTM Test Methods

E691 Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method

2.2 *ISO Standard:*

ISO 4625 Binders for paints and varnishes—Determination of softening point—Ring-and-ball method<sup>3</sup>

## 3. Summary of Test Method

3.1 These test methods are for the determination of the softening point—the temperature at which a disk of the resin held within a horizontal ring is forced downward a distance of 25.4 mm (1.00 in.) under the weight of a standard steel ball, as the specimen is heated at 5 °C/min. in a specified liquid bath.

## 4. Significance and Use

4.1 For hydrocarbon resins and rosin based resins, softening does not take place at a definite temperature. As the temperature rises, these materials gradually change from brittle solids or very viscous liquids to less viscous liquids. For this reason, determination of the softening point must be made by a fixed, arbitrary, and closely defined method if the results obtained are to be comparable.

## 5. Sample Preparation

5.1 *Preparation of Sample by the Pour Method:* This procedure is suitable for resins that can be heated and poured without adverse effect on the softening point.

5.1.1 Select a sample representative of the material to be tested. The sample should consist of flakes, pastilles, or broken lumps. Avoid inclusion of finely divided material or dust.

5.1.2 Select a quantity of resin having a volume at least twice that necessary to fill the desired number of rings, and melt it in a clean container, using an oven, hot plate, sand bath or oil bath to prevent local overheating. If necessary, stir slowly, taking care to avoid incorporating air bubbles in the

<sup>3</sup> Available from American National Standards Institute (ANSI), 25 W. 43rd St., 4th Floor, New York, NY 10036, <http://www.ansi.org>.

sample. Melt the sample completely, but do not heat it above a temperature necessary to pour the material readily. The time from the beginning of heating to pouring should not exceed 15 min.

5.1.3 For materials that tend to crack or shrink in the ring on cooling, immediately before filling the ring, preheat the ring to approximately the temperature at which the material is to be poured. The ring, while being filled, should rest **bottom down** (see Fig. 1(a)) on a suitable metal surface. Pour the sample into the ring so as to leave an excess on cooling. After cooling a minimum of 30 min, trim off the excess resin from the top and outside of the ring. To remove excess resin from the top, cut the excess off cleanly with a heated knife or spatula, or grasp the ring in a pair of tongs and draw the top surface quickly and firmly over the surface of a heated plate.

NOTE 1—If the determination is repeated, use a clean container and a fresh sample.

5.2 Preparation of Sample by the Powder Method: This procedure is suitable for high softening-point materials that cannot be heated and poured without adverse effects on the softening point. See Appendix X1.1, Alternate Sample Preparation Procedures.

5.3 Preparation of Samples Having a Low Softening Point (up to 35 °C (95 °F)):

5.3.1 Place a ring on a piece of aluminum foil. Pour the material to be tested into the ring, then place the foil and the filled ring on dry ice or in a freezer to cool. The material in the ring must be free of bubbles.

5.3.2 After cooling, cut and scrape off any excess material using a slightly heated spatula, then slide the ring gently from the foil. Place the ring in the supporting apparatus, and perform the softening point determination in accordance with Section 12.

6. Apparatus

6.1 Automated Ring-and-Ball Softening Point Instrument, having a test assembly consisting of: a ring holder, a metal plate, and a cover mounted on two support rods (see Fig. 1(b) and (d)), a built in digital temperature that should be standardized periodically to ensure that it meets the specifications for and gives the same readings as thermometers given in Specification E1, a digital temperature display, a heating unit and a heating-rate controller.

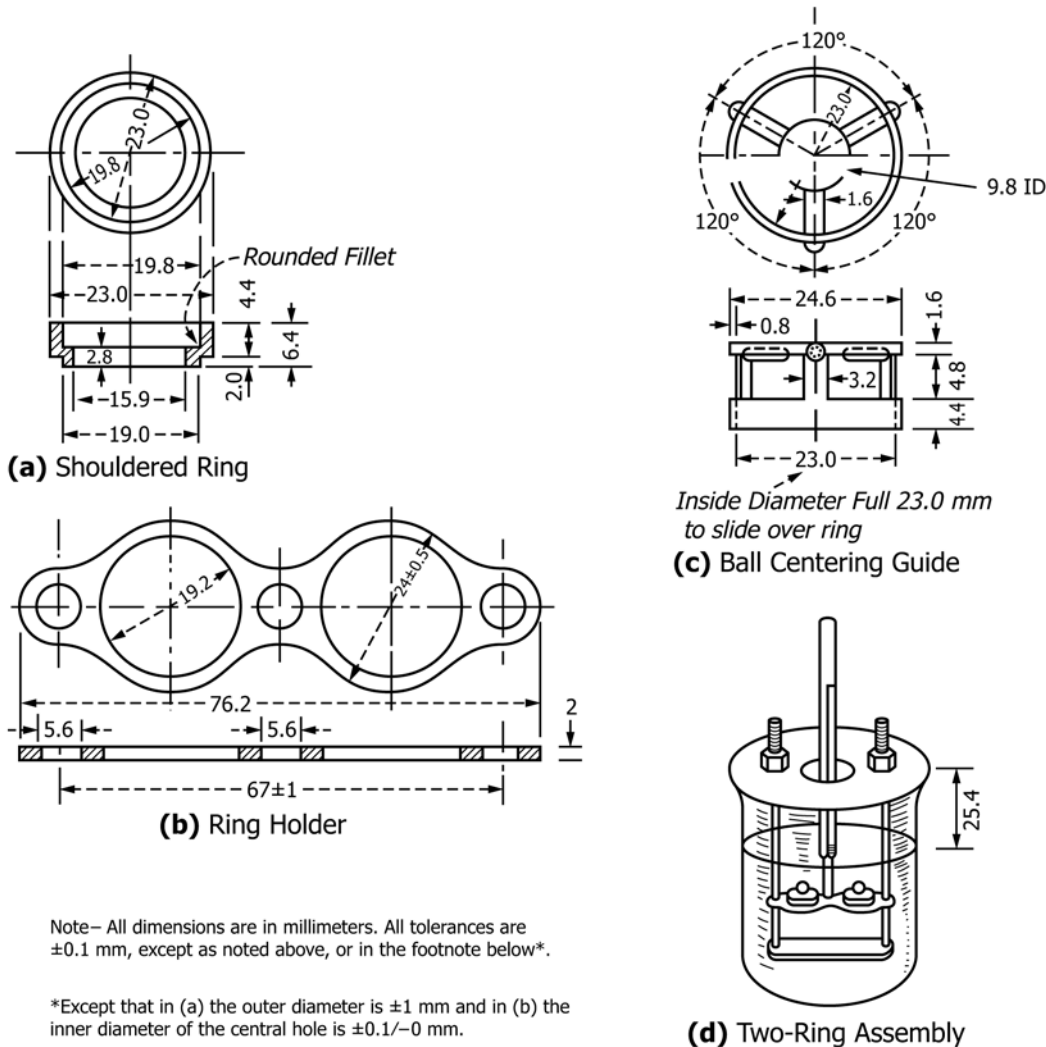


FIG. 1 Shouldered Ring, Ring Holder, Ball-Centering Guide, and Assembly of Apparatus